

(19)



(11)

EP 1 601 312 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
26.09.2007 Bulletin 2007/39

(51) Int Cl.:
A61F 2/84 (2006.01)

(21) Application number: **04712307.0**

(86) International application number:
PCT/US2004/004661

(22) Date of filing: **18.02.2004**

(87) International publication number:
WO 2004/075792 (10.09.2004 Gazette 2004/37)

(54) **STENT DELIVERY SYSTEM WITH A BALLOON CATHETER SURROUNDED BY A ROTATING SHEATH**

EINFÜHRSYSTEM FÜR EINEN STENT MIT EINEM BALLON MIT DREHBARER HÜLLE

SYSTEME DE POSE DE STENT COMPRENANT UN CATHETER A BALLONNET ENTOURE D'UNE
GAINE ROTATIVE

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR**

(30) Priority: **27.02.2003 US 375689**

(43) Date of publication of application:
07.12.2005 Bulletin 2005/49

(73) Proprietor: **Boston Scientific Limited
St. Michael, Barbados, West Indies (BB)**

(72) Inventor: **EIDENSCHINK, Tracee
Wayzata, Minnesota 55391 (US)**

(74) Representative: **Hauck Patent- und Rechtsanwälte
Postfach 11 31 53
20431 Hamburg (DE)**

(56) References cited:
**WO-A-03/017872 US-A- 5 397 305
US-A1- 2002 072 755**

EP 1 601 312 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

Description of the Related Art

[0001] Stent systems are widely used in the treatment of stenoses. Intravascular stents are used in coronary, renal, and carotid arteries, for example, to maintain an open passage through the artery. In patients whose coronary heart disease consists of focal lesions, stents have proven effective. For example, where only a single coronary artery is clogged or where there are short blockages in more than a single artery, stents have been used with a great amount of success. An intravascular stent may be positioned in a clogged artery by a catheter and is often set in place by inflating a balloon upon which the stent is mounted. This expands the diameter of the stent and opens the previously clogged artery. The balloon is then deflated and removed from the patient while the stent retains an open passage through the artery.

[0002] Treatment at bifurcation sites has been difficult. Although efforts have been made to use a stent at bifurcations, these sites have previously been problematic to treat. The specialty stents designed for bifurcations generally need specific alignment, radially as well as longitudinally. For example, U.S. Patent No. 5,749,825 is representative of a catheter system that treats stenoses at an arterial bifurcation.

[0003] A stent having different diameters has been proposed to allow placement in both a primary passage, such as an artery, and a secondary passage, such as a side branch artery. Additionally, these stents generally have a circular opening which allows for unimpeded blood flow into the side branch artery. However, problems are still encountered in orienting the stent relative to the side branch at the bifurcation of the primary and secondary passages.

[0004] Many current devices rely on either passive torque (e.g., pushing the stent forward and allowing the stent that is fixed on the guide wire/balloon to passively rotate itself into place) or creating torque from outside of the patient to properly orient the medical device in the passage. These devices and methods of achieving proper angular orientation have not been shown to be effective in properly placing and positioning the stent. As will be appreciated and understood by those skilled in the art, improper placement of the stent with respect to its rotational or circumferential orientation, or its longitudinal placement, could lead to obstruction of the side branch passage. It is important to properly position or center an opening formed in the bifurcated stent with the secondary passage to maximize flow therethrough.

[0005] Thus, a need exists for effectively treating stenosed passage bifurcations. This need includes more precise and exact longitudinal placement and rotational circumferential orientation of the stent.

[0006] Many commercially available devices do not

maintain side branch access at the time of stent deployment. This results in the potential for plaque shift and occlusion of the secondary passage.

[0007] It would also be advantageous if stents could be placed across the side branch while wire position is maintained thereby helping to protect and secure further access to the side branch.

[0008] US 2002/0072755 discloses a stent deployment catheter where the stent is placed on a balloon which is rotatable round the catheter shaft.

[0009] Without limiting the scope of the invention a brief summary of some of the claimed embodiments of the invention is set forth below. Additional details of the summarized embodiments of the invention and/or additional embodiments of the invention may be found in the Detailed Description of the Invention below.

[0010] A brief abstract of the technical disclosure in the specification is provided. The abstract is not intended to be used for interpreting the scope of the claims.

BRIEF SUMMARY OF THE INVENTION

[0011] Some embodiments of the present invention include a freely rotating deployment assembly for a stent assembly maintaining side branch access and protection.

[0012] The present invention contemplates an apparatus that improves the orientation of a stent by providing a more exact placement of the stent relative to the side branch passage. This, in turn, may lead to better protection of the side branch passage.

[0013] The invention includes a medical device with a balloon catheter shaft and a rotating sheath. In some embodiments the catheter shaft has a first guide wire lumen therethrough and an inflation lumen extending from a proximal region of the catheter shaft to a distal region of the catheter shaft.

[0014] In at least one embodiment at least a portion of the distal region of the catheter shaft has a balloon disposed about it.

[0015] In some embodiments no portion of the sheath is more than about 5 centimeters proximal to the most proximal portion of the balloon.

[0016] In at least some embodiments a stent may be situated about the sheath.

[0017] In at least one embodiment a second guide wire lumen with a portion disposed under the stent contains a portion of a second guide wire.

[0018] In some embodiments the stent is self expanding. In some embodiments the stent is balloon expandable. In some embodiments the stent is made of shape memory material.

[0019] In some embodiments the sheath is constructed such that it is radially expandable.

[0020] In some embodiments the sheath is constructed such that the stent may be crimped onto the sheath.

[0021] In some embodiments the sheath is constructed of at least one homogeneous layer.

[0022] In some other embodiments the sheath has a low friction inner surface. In other embodiments a friction reducing substance is placed between the sheath and the inner balloon. In other embodiments a friction reducing substance is placed between an outer balloon and the inner balloon.

[0023] In some embodiments the sheath is constructed of a soft durometer polymer.

[0024] In at least one embodiment the sheath is constructed of multiple layers.

[0025] In at least one embodiment at least one of the layers is constructed of a first material having different properties from a second material found in at least one other layer.

[0026] In some other embodiments an inner layer constructed of a low friction material is in contact with the balloon. Materials such as PTFE and HDPE are used in some embodiments.

[0027] In some embodiments an outer layer of a soft durometer polymer suitable for securing the stent to the sheath is used.

[0028] In some other embodiments the sheath is made of a shape memory material so it shrinks back down for withdrawal.

[0029] In some other embodiments the sheath rotates freely.

[0030] In at least one other embodiment the longitudinal movement of the sheath relative to the balloon catheter shaft is limited with a safety tether. The safety tether can be a pull wire outside either guidewire lumen or it can be inside the second wire lumen.

[0031] In some embodiments the catheter balloon has at least one balloon cone distally offset from the distal most portion of the sheath or proximally offset from the proximal most portion of the sheath.

[0032] In some embodiments the assembly has marker bands located about the balloon catheter shaft. In some embodiments the marker bands have a greater diameter than the cross-sectional diameter of the sheath thereby limiting longitudinal movement of the sheath relative to the balloon catheter shaft. In some embodiments at least one marker band has a radiopaque portion.

[0033] In some embodiments a rotating collar is positioned about the second wire lumen and the balloon catheter shaft. In other such embodiments a first longitudinal lock is positioned about the second wire lumen and proximal to the rotating collar, and a second longitudinal lock is positioned about the balloon catheter shaft and distal to the rotating collar such that the longitudinal position of the sheath and collar is maintained.

[0034] In some embodiments the medical device has a hypotube engaged to the sheath at the distal end of the hypotube and engaged to the collar at the proximal end of the hypotube.

[0035] In some embodiments the hypotube is spiral cut. In some embodiments the hypotube comprises stainless steel. In some embodiments the hypotube comprises a polymer.

[0036] In some embodiments the proximal end of the hypotube is disposed in a second guide wire lumen of the collar.

[0037] In some embodiments the proximal end of the hypotube is engaged to an outside surface of the collar.

[0038] In some embodiments the sheath has a length that is substantially the same as the length of the catheter balloon.

[0039] In some embodiments the balloon has a body portion with a cone portion distal to the body portion and a cone portion proximal to the body portion, and the sheath is disposed about the body portion and has a length substantially the same as the length of the body portion of the catheter balloon.

[0040] In some embodiments the length of the sheath is no greater than 2 centimeters longer than the length of the balloon.

[0041] In some embodiments the sheath extends distally from a location proximal to the proximal end of the catheter balloon. In some embodiments the sheath extends distally from a location equal to or less than 2 centimeters proximal to the proximal end of the catheter balloon.

[0042] In some embodiments the assembly provides for proper orientation relative to the side branch, side branch protection with the guide wire during stent deployment, proper placement of the stent both longitudinally and circumferentially, and reduction in the incidence of tangled wires.

[0043] An embodiment not covered by the scope of the claims is also shown where an outer balloon may replace the sheath of the above embodiments. The outer balloon in such instances may have the same qualities as the sheath as described in the embodiments above.

[0044] These and other embodiments which characterize the invention are pointed out with particularity in the claims annexed hereto and forming a part hereof. However, for a better understanding of the invention, its advantages and objectives obtained by its use, reference should be made to the drawings which form a further part hereof and the accompanying descriptive matter, in which there is illustrated and described a embodiments of the invention.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING(S)

[0045] A detailed description of the invention is hereafter described with specific reference being made to the drawings.

FIG. 1 is a perspective view of an embodiment of the invention wherein the assembly is shown in a pre-deployment configuration.

FIGS. 2a-d are cross-sectional views of sheath configurations.

FIG. 3 is a perspective view of an embodiment of the invention wherein the assembly is shown having bal-

loon cones on the balloon.

FIG. 4 is a perspective view of an embodiment of the invention wherein the assembly is shown having large diameter marking bands.

FIG. 5 is a perspective view of an embodiment of the invention wherein the assembly is shown illustrating the tether attachment and also the rotating collar and longitudinal locks.

FIG. 6 is a cross-sectional view of the rotating collar from view A-A of Fig. 5.

FIG. 7 is a perspective view of an embodiment of the invention wherein the assembly is shown having an outer balloon in place of the sheath.

FIG. 8 is a perspective view of a catheter balloon illustrating the body portion and the cone portions of the catheter balloon.

FIG. 9 is a perspective view of an embodiment of the invention wherein the assembly is shown having a hypotube which is disposed in the second guide wire collar lumen.

FIG. 10 is a perspective view of an embodiment of the invention wherein the assembly is shown having a hypotube engaged to the collar.

DETAILED DESCRIPTION OF THE INVENTION

[0046] While this invention may be embodied in many different forms, there are described in detail herein specific embodiments of the invention. This description is an exemplification of the principles of the invention and is not intended to limit the invention to the particular embodiments illustrated.

[0047] For the purposes of this disclosure, like reference numerals in the figures shall refer to like features unless otherwise indicated.

[0048] Referring now to the drawings which are for the purposes of illustrating embodiments of the invention only and not for purposes of limiting same, in at least one embodiment of the invention, an example of which is shown in FIG. 1, an assembly 10 is shown. The assembly is designed to provide better axial and longitudinal positioning of a stent in a bifurcation site. The assembly 10 has an outer catheter shaft 14 with an inner catheter shaft 16 defining a wire lumen 17 and an inflation lumen 18 extending from a proximal region of the catheter to a distal region of the catheter. The inner lumen 17 is constructed such that it can be disposed about a guide wire which provides means for guiding the catheter to the treatment site. The inflation lumen 18 provides a passage for the inflating fluid to both inflate and deflate the catheter balloon 20. The catheter balloon 20 is sealingly engaged at its proximal end 20a to the outer shaft 14 and is sealingly engaged at its distal end 20b to the inner shaft 16.

[0049] A sheath 22 is disposed about the balloon 20. The sheath is designed to be freely rotatable about the balloon. The sheath 22 can be constructed of a low friction material such as PTFE or HDPE which allows the sheath to freely rotate about the balloon 20. In some em-

bodiments at least a portion of balloon 20 may include a coating of one or more low friction materials or include one or more low friction materials in its construction. In some embodiments the assembly 10 may be used to deliver a stent 24 to a vessel bifurcation. In such embodiments a stent 24 is disposed about and crimped upon the sheath 22. The rotatability of the sheath 22 allows a stent 24 disposed thereabout to be freely rotated within a vessel or lumen to allow one or more openings of the stent to be aligned with a branch of the bifurcation.

[0050] It should be noted that the sheath can also have multiple layers. An outer layer 22a of the sheath 22 may be constructed of a softer material than that of the material used in constructing the inner layer 22b of the sheath 22. The softer outer layer will provide improved stent securement upon crimping of the stent 24. In one embodiment, a soft polymer is one with a durometer hardness of less than about 55D. Possible materials for the outer layer are a polymer like PEBAX (55D), a urethane, etc. The low friction inner layer 22b can be constructed of PTFE or HDPE.

[0051] A second shaft 25 defining the second wire lumen 26 is engaged along a portion of the sheath 22. The sheath itself can also define the second wire lumen 26. Rotational torque indicated by arrows 27 may be applied to the sheath 22 when the catheter is advanced to the bifurcation site in the following manner:

[0052] In some embodiments of the assembly 10 is advanced along two guide wires 29 and 44 as shown in Fig. 5. The first guidewire 29 is positioned in the primary passage or branch vessel and is disposed inside the inner lumen 17 of the catheter shaft 14. The second guidewire 44 diverges from the first guidewire 29 upon passage into the secondary branch in the region of the bifurcation. The inner lumen 17 of the stent delivery assembly 10 is disposed about the guidewire 29 in the primary passage while the second wire lumen 26 of the stent delivery assembly 10 is disposed about the second guidewire which extends into the secondary passage of the bifurcation. As the stent delivery assembly 10 approaches the bifurcation, the sheath 22 which is engaged to the second wire lumen 26 will then rotate so as to be aligned with the side wall passage at the bifurcation. A tether 34 can also be added in order to limit the distal movement of the sheath 22 in relation to the inner shaft 16. The tether 34 can be attached directly to the sheath at tether engagement point 11.

[0053] The sheath or the outside balloon, as illustrated in Fig. 7, substantially freely rotates about the inner shaft 16 and/or balloon 20. The sheath or outside balloon may rotate less than a single degree or over 360 degrees in order to align at least one of the openings in the stent with a side branch lumen at a bifurcation site.

[0054] In Figs. 2a-2c cross-sections of different embodiments of the shown sheath 22 in the unexpanded state prior to the delivery of the stent are illustrated. The second shaft 25 defining the second wire lumen 26 is engaged to the sheath 22. In another embodiment such

as is shown in Fig. 2a a sheath having a second shaft 25a is attached to the sheath 22a. In a balloon expandable delivery system the sheath 22a is arranged in a coil-like structure before deployment of the stent. During delivery of the stent, the sheath 22a uncoils. In another embodiment such as is shown in Fig. 2b a sheath having a clam shell cross-section is shown in the unexpanded state. The second shaft 25b is engaged to the sheath at an end of the sheath 22b. In another embodiment such as is shown in Fig. 2c a sheath prior to delivery of the stent has a cross-section in the unexpanded state shaped in an accordion-like structure. The folds 28 in the unexpanded state can be pressed down or wrapped as shown in Fig. 2d.

[0055] In some cases it may be desirable to provide external protection of the sheath to prevent the sheath from being longitudinally displaced during advancement of the catheter and/or delivery of the stent. In Fig. 3 an embodiment is shown wherein the balloons end portions or cones 30 are provided with a diameter about the inner catheter shaft 16 greater than the cross-sectional diameter of the sheath 22. Thus, as a result of the position of the cones 30 about the ends of the sheath 22 the longitudinal movement of the sheath 22 relative to the inner catheter shaft 16 is limited. In another embodiment shown in Fig. 4, the sheath is protected by the inclusion of one or more hubs, protrusions, marker bands 32, etc. with a diameter sufficient to prevent the sheath from moving in a longitudinal direction. These marker bands 32 act like a dam on each end of the sheath 22 by forcing portions of the balloon radially outward such that these portions of the balloon 20 have a greater diameter than the diameter of the sheath 22. In the embodiments shown in Figs. 3 and 4 the stent 24 in either or both the expanded and the unexpanded conditions may have a greater diameter than the cones 30 while the sheath 22 does not.

[0056] In Fig. 5 an embodiment of the invention is shown wherein the assembly is provided with a safety tether 34. The tether 34 (shown in this figure overlapping the second guide wire 44) can be a simple pull wire that runs along the length of the catheter 10 and engages the sheath 22. The tether 34 can extend into the second wire lumen 26 and thereby engage the sheath 22 or the second shaft 25 at an engagement point 35. The safety tether 34 can also attach to the sheath 22 directly as shown in Fig. 1 at tether engagement point 11.

[0057] As shown in the cut away portion of Fig. 5 and in Fig. 6 the catheter 10 may include a rotating collar 36 having a second guide wire collar lumen 38 and an outer catheter shaft collar lumen 39 which is disposed about the outer catheter shaft 14. A distal longitudinal lock 40 disposed about the catheter shaft and both adjacent and distal to the collar 36 limits longitudinal movement of the collar 36. The distal longitudinal lock 40 has a diameter greater than the diameter of the outer catheter shaft collar lumen 39. The proximal longitudinal lock 42 disposed about a second guide wire 44 has a greater diameter than the second guide wire collar lumen 38, thus limiting

the wire 44 from distal movement beyond the point when the proximal longitudinal lock 42 comes into contact with the second guide wire collar lumen 36.

[0058] In Fig. 7 an outer balloon 46 which rotates around the inner balloon 20 is used in place of a sheath 22. In such embodiments not included in the scope of the claims the outer balloon 46 is sealed at first end 48 and second end 50 of the catheter 10. Balloon movement stoppers 52 limit longitudinal movement of the balloons. The outer balloon 46 can be constructed of a low friction material such as PTFE or HDPE which allows the outer balloon 46 to freely rotate about the inner balloon 20. The stent 24 is disposed about and crimped upon the outer balloon 46. It should be noted that the outer balloon can also have multiple layers. An outer layer of the outer balloon 46 may be constructed of a softer material than that of the material used in constructing the inner layer of the outer balloon 46. Where the balloon is provided with a softer outer layer, the softer outer layer may provide improved stent securement upon crimping of the stent 24. In one embodiment, a soft polymer is one with a durometer hardness of less than about 55D. Possible materials for the outer layer are a polymer like PEBAX (55D), a urethane, etc. The low friction inner layer of the outer balloon 46 can be constructed of PTFE or HDPE and/or other suitable materials.

[0059] In the embodiment shown in Fig. 7 the outer balloon 46 is rotatable about the inner balloon 20. Gap 58 (shown on only one end, first end 48) acts as a friction reducing mechanism between outer balloon seal site 54 and inner balloon seal site 56. Gap 58 includes a friction reducing fluid, a low friction material, a bearing system, etc., or any combination thereof.

[0060] In the embodiment shown in Fig. 8 the cones 30 and body portion 60 of the catheter balloon 20 are shown. In some embodiments of the invention the sheath 22 is of the substantially same length as the body portion 60 of the catheter balloon 20. In some embodiments the sheath 22 is disposed substantially on the body portion 60 of the balloon 20. In other embodiments the sheath 22 extends longitudinally such that a portion of the sheath 22 is disposed about at least one of the cone portions 30.

[0061] In the embodiments of Figs. 9 and 10 a hypotube 64 is engaged to the collar 38 and the sheath 22. The hypotube 64 may comprise stainless steel or it may comprise a polymer. The hypotube 64 may be constructed to be spiral cut. The spiral cut 65 may include scoring, cutting, indenting, perforating, puncturing, etc. The hypotube 64 may thus be firm in the longitudinal direction but may also be flexible due to the spiral cut

[0062] Figs. 9 and 10 also illustrate embodiments having both the proximal longitudinal lock 42 and the distal longitudinal lock 40 disposed about the outer catheter shaft 14 rather than as shown in Figs. 5 and 6 wherein one longitudinal lock is disposed about the guidewire 44 or safety tether 34.

[0063] Fig. 9 specifically illustrates an embodiment wherein the hypotube 64 is disposed in the second guide

wire collar lumen 38. The hypotube 64 may be disposed in only a portion of the second guide wire collar lumen 38. The collar 36 rotates along with the sheath 22 and thus may rotate simultaneously and/or with equal degrees of rotation. In Fig. 10 the hypotube 64 is engaged to an outside surface of the collar 36. In both Figs. 9 and 10 engagement of the hypotube 64 to the collar 36 and sheath 22 can be through chemical welding, heat welding, laser welding, chemical bonding, adhesives, fastening devices, etc.

[0064] The invention has been described with reference to the embodiments. Obviously, modifications and alterations will occur to others upon a reading and understanding of this specification. For example, the illustrated embodiments use a balloon to expand the stent although, as briefly noted above, a self expanding or self deploying stent can be used without departing from the features of the present invention. Likewise, using a fixed wire on the distal end of the apparatus is also recognized as being consistent with the features of the present invention. Moreover, the embodiments describe a side branch hypotube, either split or unsplit, that is associated with the side branch guide wire. It will be further appreciated that the side branch guide wire could be carried and/or released in a variety of other ways. The invention is intended to include all such modifications and alterations thereof.

[0065] The above disclosure is intended to be illustrative and not exhaustive. This description will suggest many variations and alternatives to one of ordinary skill in this art. All these alternatives and variations are intended to be included within the scope of the claims where the term "comprising" means "including, but not limited to". Those familiar with the art may recognize other equivalents to the specific embodiments described herein which equivalents are also intended to be encompassed by the claims.

Claims

1. A medical device comprising:

a balloon catheter shaft (14) having a catheter balloon (20), the catheter balloon having a length, a sheath (22) disposed about the catheter balloon, **characterised by** the sheath being substantially freely rotatable about the catheter balloon.

2. The medical device of claim 1, wherein no portion of the sheath (22) is more than about 5 centimeters proximal to a most proximal portion of the balloon (20).

3. The medical device of claim 1, wherein the balloon catheter shaft (14) defines a first guide wire lumen (17), and the sheath (22) at least partially defines a

second guide wire lumen (26).

4. The medical device of claim 1, wherein the sheath (22) is at least partially constructed of multiple layers, an inner layer (22b) of the sheath being in contact with the balloon (20) and constructed of at least one low friction material having different properties from an outer layer (22a) of a soft durometer polymer suitable for securing a stent (24) to the sheath (22).

5. The medical device of claim 1, wherein the sheath (22) has an expanded state when the balloon (20) is in an expanded condition and an unexpanded state when the balloon is in an unexpanded condition, the sheath rotating substantially freely about the balloon when in the unexpanded state or the expanded state.

6. The medical device of claim 3, further comprising at least one pullwire (34) positioned external of at least one of the guide wire lumens.

7. The medical device of claim 3, wherein a rotating collar (36) is positioned about the second wire lumen (26) and the balloon catheter shaft (14).

8. The medical device of claim 7, wherein a first longitudinal lock (42) is positioned about the second wire lumen (26) and proximal to the rotating collar (36), and a second longitudinal lock (40) is positioned about the balloon catheter shaft (14) and distal to the rotating collar (36) such that the longitudinal position of the sheath (22) and collar (36) is maintained.

9. The medical device of claim 7, wherein a hypotube (64) having a distal end and a proximal end is engaged to the sheath (22) at the distal end of the hypotube and to the collar (38) at the proximal end.

10. The medical device of claim 1 wherein the sheath has a length (22) that is substantially the same as the length of the catheter balloon (20).

11. The medical device of claim 1 wherein the balloon (20) has a body portion (60) with a cone (30) portion distal to the body portion (60) and a cone portion (30) proximal to the body portion (60), the sheath (22) disposed about the body portion (60) and having a length substantially the same as the length of the body portion (60) of the catheter balloon.

Patentansprüche

1. Medizinisches Instrument, umfassend:

einen Ballonkatheterschaft (14), der einen Katheterballon (20) aufweist, wobei der Katheter-

- ballon eine Länge, eine Hülle (22), die um den Katheterballon angeordnet ist, aufweist, **dadurch gekennzeichnet, dass** die Hülle im Wesentlichen um den Katheterballon frei drehbar ist.
2. Medizinisches Instrument nach Anspruch 1, bei dem kein Abschnitt der Hülle (22) mehr als ungefähr 5 Zentimeter proximal zu einem am meisten proximalen Abschnitt des Ballons (20) liegt.
 3. Medizinisches Instrument nach Anspruch 1, bei dem der Ballonkatheterschaft (14) einen ersten Führungsdraht Hohlräum (17) bestimmt und die Hülle (22) teilweise einen zweiten Führungsdraht Hohlräum (26) bestimmt.
 4. Medizinisches Instrument nach Anspruch 1, bei dem die Hülle (22) mindestens teilweise aus mehreren Schichten aufgebaut ist, wobei eine innere Schicht (22b) der Hülle den Ballon (20) berührt und aus mindestens einem Werkstoff mit geringer Reibung aufgebaut ist, der unterschiedliche Eigenschaften aufweist, von einer äußeren Schicht (22a) eines weichen Durometer-Polymers, das geeignet ist, um einen Stent (24) an der Hülle (22) zu sichern.
 5. Medizinisches Instrument nach Anspruch 1, bei dem die Hülle (22) einen entfalteten Zustand aufweist, wenn sich der Ballon (20) in einem entfalteten Zustand befindet, und einen nicht entfalteten Zustand, wenn sich der Ballon in einem nicht entfalteten Zustand befindet, wobei die Hülle im Wesentlichen frei um den Ballon dreht, wenn sie sich im nicht entfalteten Zustand oder im entfalteten Zustand befindet.
 6. Medizinisches Instrument nach Anspruch 3, überdies umfassend mindestens eine Reißleine (34), die außerhalb mindestens eines der Führungsdraht Hohlräume positioniert ist.
 7. Medizinisches Instrument nach Anspruch 3, bei dem eine Drehmanschette (36) um den zweiten Draht Hohlräum (26) und den Ballonkatheterschaft (14) positioniert ist.
 8. Medizinisches Instrument nach Anspruch 7, bei dem eine erste in Längsrichtung verlaufende Verriegelung (42) um den zweiten Draht Hohlräum (26) und proximal zur Drehmanschette (36) positioniert ist und eine zweite in Längsrichtung verlaufende Verriegelung (40) um den Ballonkatheterschaft (14) und distal zur Drehmanschette (36) positioniert ist, so dass die in Längsrichtung verlaufende Position der Hülle (22) und der Manschette (36) beibehalten wird.
 9. Medizinisches Instrument nach Anspruch 7, bei dem einen Hypotube (64), das ein distales Ende und ein proximales Ende aufweist, mit der Hülle (22) an dem distalen Ende des Hypotubes und an der Manschette (38) an dem proximalen Ende in Eingriff ist.
 10. Medizinisches Instrument nach Anspruch 1, bei dem die Hülle eine Länge (22) aufweist, die im Wesentlichen die gleiche ist, wie die Länge des Katheterballons (20).
 11. Medizinisches Instrument nach Anspruch 1, bei dem der Ballon (20) einen Körperabschnitt (60) mit einem kegelförmigen Abschnitt (30) distal zum Körperabschnitt (60) und einem kegelförmigen Abschnitt (30) proximal zum Körperabschnitt (60) aufweist, die Hülle (22) um den Körperabschnitt (60) angeordnet ist und eine Länge aufweist, die im Wesentlichen die gleiche ist, wie die Länge des Körperabschnitts (60) des Katheterballons.

Revendications

1. Dispositif médical comprenant :

une tige (14) de cathéter à ballonnet ayant un ballonnet (20) de cathéter, le ballonnet de cathéter ayant une longueur, une gaine (22) disposée autour du ballonnet de cathéter, **caractérisé par** la gaine qui peut tourner de manière sensiblement libre autour du ballonnet de cathéter.

2. Dispositif médical selon la revendication 1, dans lequel aucune partie de la gaine (22) n'est supérieure à environ 5 centimètres de manière proximale à la partie la plus proximale du ballonnet (20).

3. Dispositif médical selon la revendication 1, dans lequel la tige (14) de cathéter à ballonnet définit une première lumière (17) de fil guide et la gaine (22) définit au moins partiellement une seconde lumière (26) de fil guide.

4. Dispositif médical selon la revendication 1, dans lequel la gaine (22) est au moins partiellement construite avec plusieurs couches, une couche interne (22b) de la gaine étant en contact avec le ballonnet (20) et construite avec au moins un matériau à faible frottement ayant des propriétés différentes d'une couche externe (22a) d'un polymère à duromètre souple approprié pour fixer un stent (24) sur la gaine (22).

5. Dispositif médical selon la revendication 1, dans lequel la gaine (22) a un état expansé lorsque le ballonnet (20) est dans une condition expansée et un état non expansé lorsque le ballonnet est dans une condition non expansée, la gaine tournant de ma-

nière sensiblement libre autour du ballonnet lorsqu'il est dans l'état non expansé ou dans l'état expansé.

6. Dispositif médical selon la revendication 3, comprenant en outre au moins un fil de traction (34) positionné à l'extérieur d'au moins l'une des lumières de fil guide. 5

7. Dispositif médical selon la revendication 3, dans lequel un collier rotatif (36) est positionné autour de la seconde lumière de fil (26) et la tige (14) de cathéter à ballonnet. 10

8. Dispositif médical selon la revendication 7, dans lequel un premier verrouillage longitudinal (42) est positionné autour de la seconde lumière de fil (26) et à proximité du collier rotatif (36) et un second verrouillage longitudinal (44) est positionné autour de la tige (14) de cathéter à ballonnet et distal par rapport au collier rotatif (36) de sorte que la position longitudinale de la gaine (22) et du collier (36) est maintenue. 15
20

9. Dispositif médical selon la revendication 7, dans lequel un hypotube (64) ayant une extrémité distale et une extrémité proximale est mis en prise sur la gaine (22) au niveau de l'extrémité distale de l'hypotube et sur le collier (38) au niveau de l'extrémité proximale. 25
30

10. Dispositif médical selon la revendication 1, dans lequel la gaine a une longueur (22) qui est sensiblement la même que la longueur du ballonnet (20) de cathéter. 35

11. Dispositif médical selon la revendication 1, dans lequel le ballonnet (20) a une partie de corps (60) avec une partie de cône (30) distale par rapport à la partie de corps (60) et une partie de cône (30) proximale par rapport à la partie de corps (60), la gaine (22) étant disposée autour de la partie de corps (60) et ayant une longueur sensiblement identique à la longueur de la partie de corps (60) du ballonnet de cathéter. 40
45

50

55

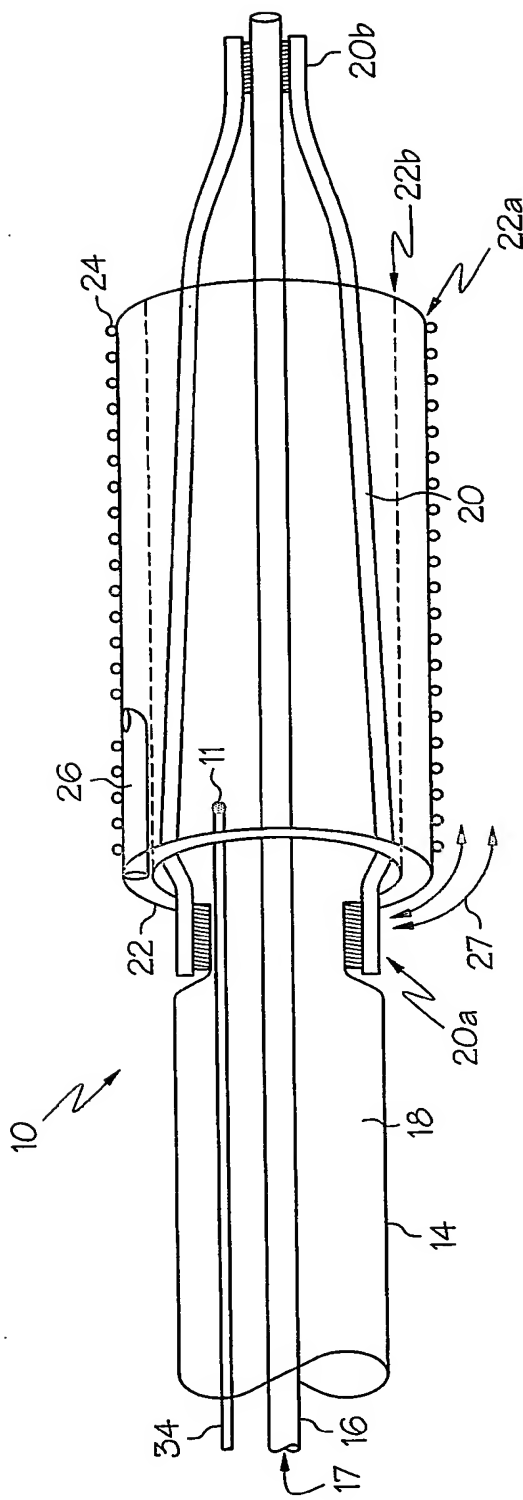


FIG. 1




FIG. 2a




FIG. 2b




FIG. 2c




FIG. 2d

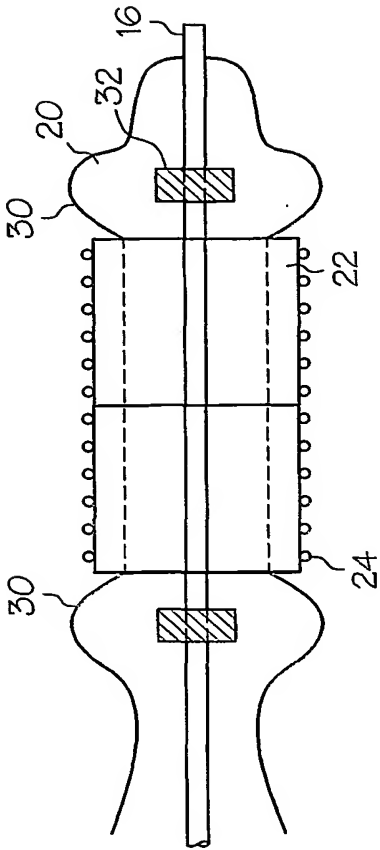


FIG. 3

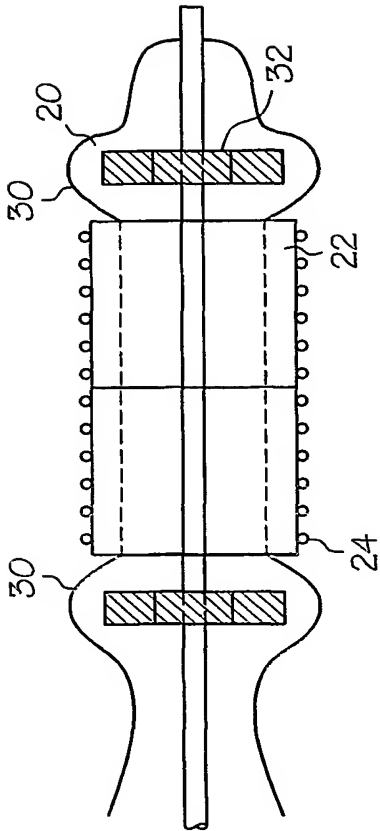


FIG. 4

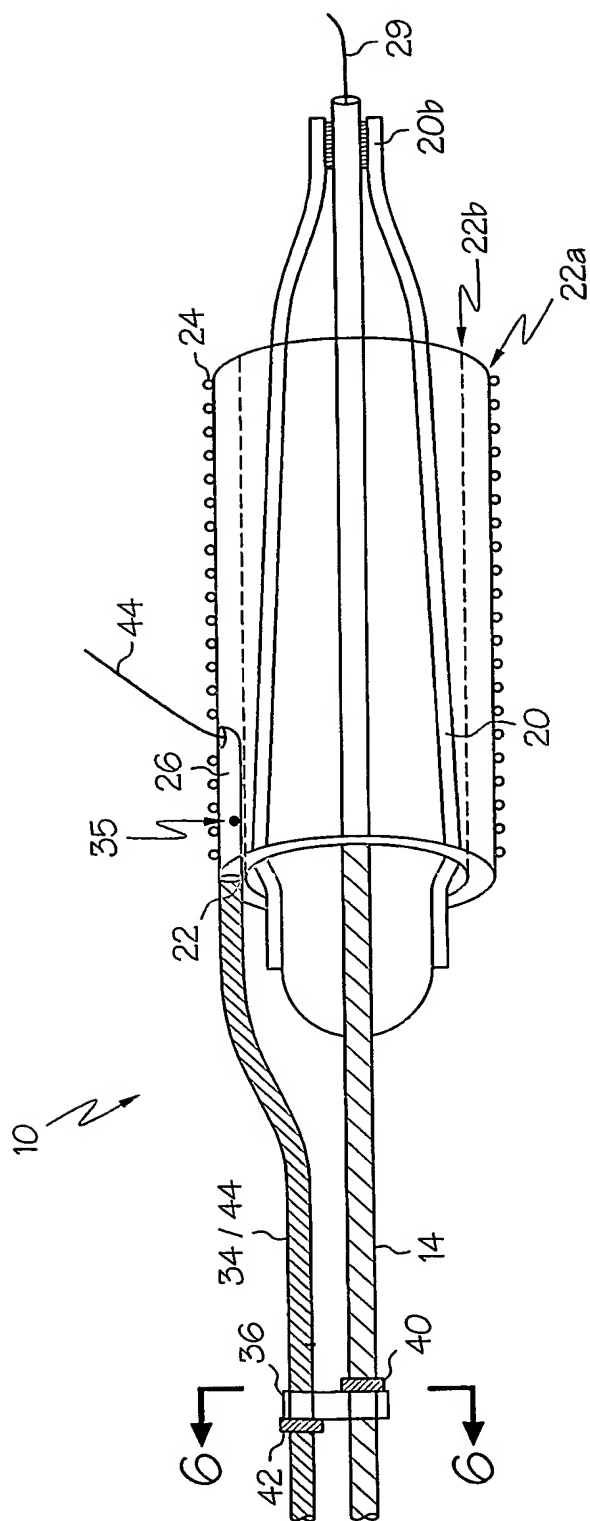


FIG. 5




FIG. 6

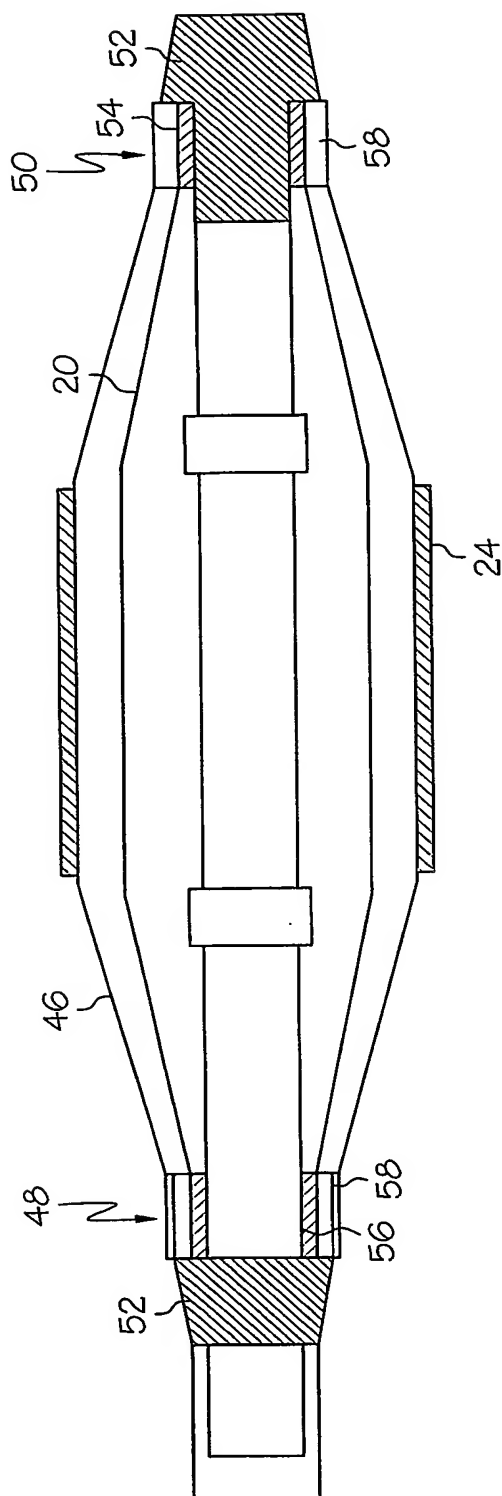


FIG. 7

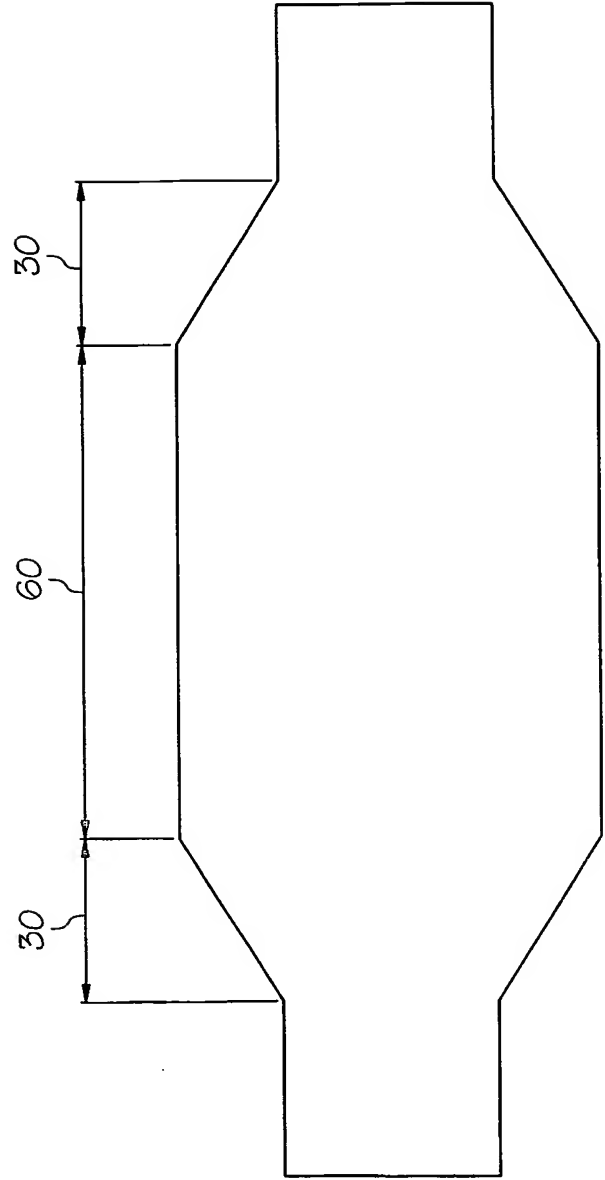


FIG. 8

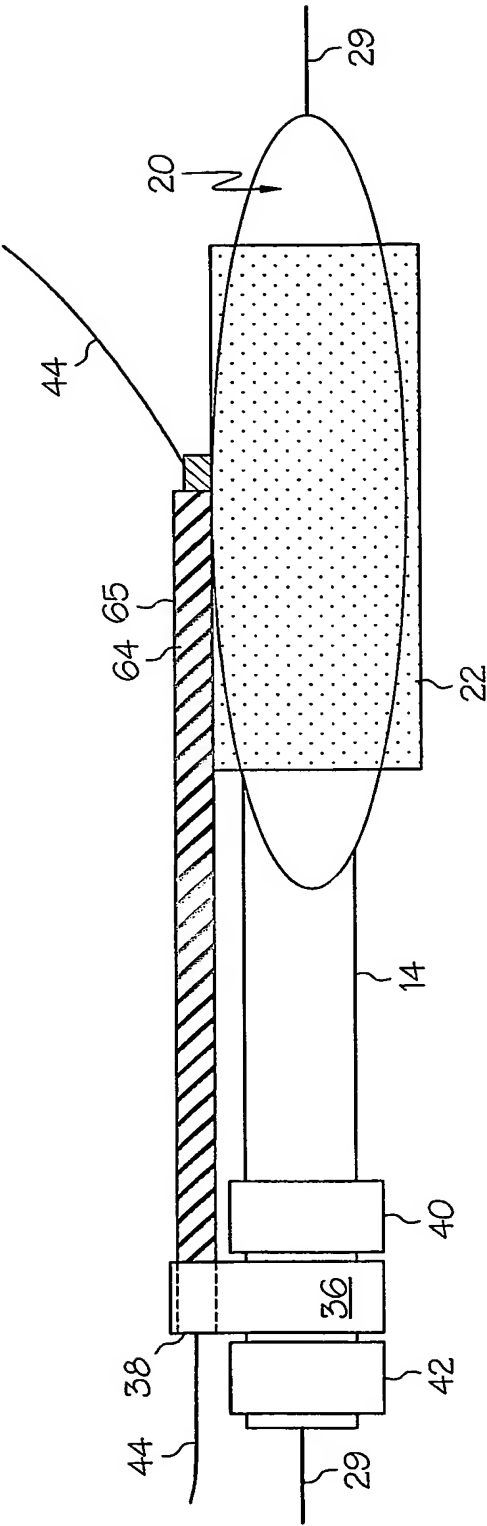


FIG. 9

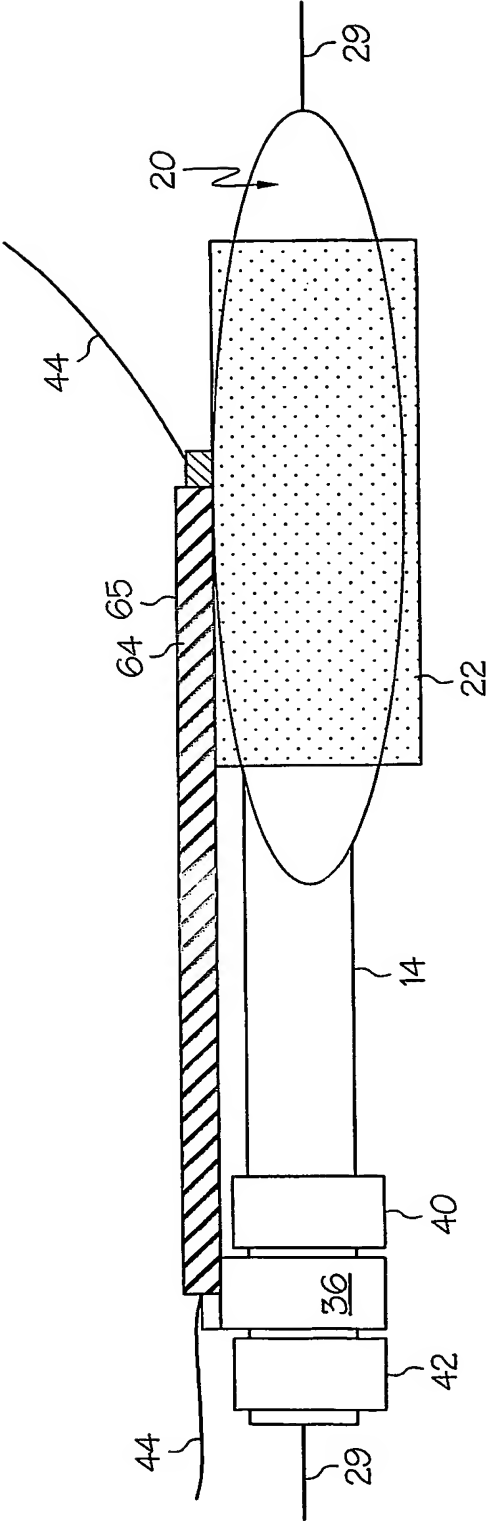


FIG. 10

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5749825 A [0002]
- US 20020072755 A [0008]